Heritage Medical Products, Inc.

SonoBed Parts Identifier

Table of Contents

Hand Controls.....2

Control Boxes.....4

Power Cords.....8

Lift Columns.....9

Actuators.....10

Foot Controls.....11

Distribution Boxes and Cords.....12

Casters.....12

Paper Roll Holder.....14

Magnetic Hanger.....14

Heritage Medical Products, Inc.

Hand Controls:

The part number for the hand controls is on the back of the hand control stamped in yellow. It can be diffilcult to read. The part number is EHA followed by numbers.

1 Function Hand Control | Part Number: EHA11-21B10N-000

2 Function Hand Control | Part Number: EHA12-21B20N-000

3 Function Hand Control | Part Number: EHA13-21B30N-000

4 Function Hand Control | Part Number: EHA14-21B40N-000

4 Function Hand Control | Part Number: EHA24-21B40N-000

5 Function Hand Control | Part Number: EHA25-21B50N-000

1 Function Hand Control | Part Number: EHA31-23M1ON-000

2 Function Hand Control | Part Number: EHA32-23M2ON-000

3 Function Hand Control | Part Number: EHA-33-23M30N-000

4 Function Hand Control | Part Number: EHA34-23M4ON-000

5 Function Hand Control | Part Number: EHA35-23M5ON-000



Heritage Medical Products, Inc.







Heritage Medical Products, Inc.

Control Boxes:

KOM Boxes





1 Function Control Box | Part Number: KOM31-20A-011

2 Function Control Box | Part Number: KOM33-20A-011

3 Function Control Box | Part Number: KOM33-20A-011

4 Function Control Box | Part Number: KOM14-020A-000

*KOM25-20A-011 Have been discontinued

Alternative control box for KOM25 replacements are VCU55 with EHA34 (4 function) or EHA35 (5 function) hand control.

Heritage Medical Products, Inc.

BCU Boxes and BCP Code




For BCU boxes we will need the BCP code also on the control box

BCU53 | Part Number: BCU-53 2L3100-0000

Heritage Medical Products, Inc.

VCU Boxes and VCP Code

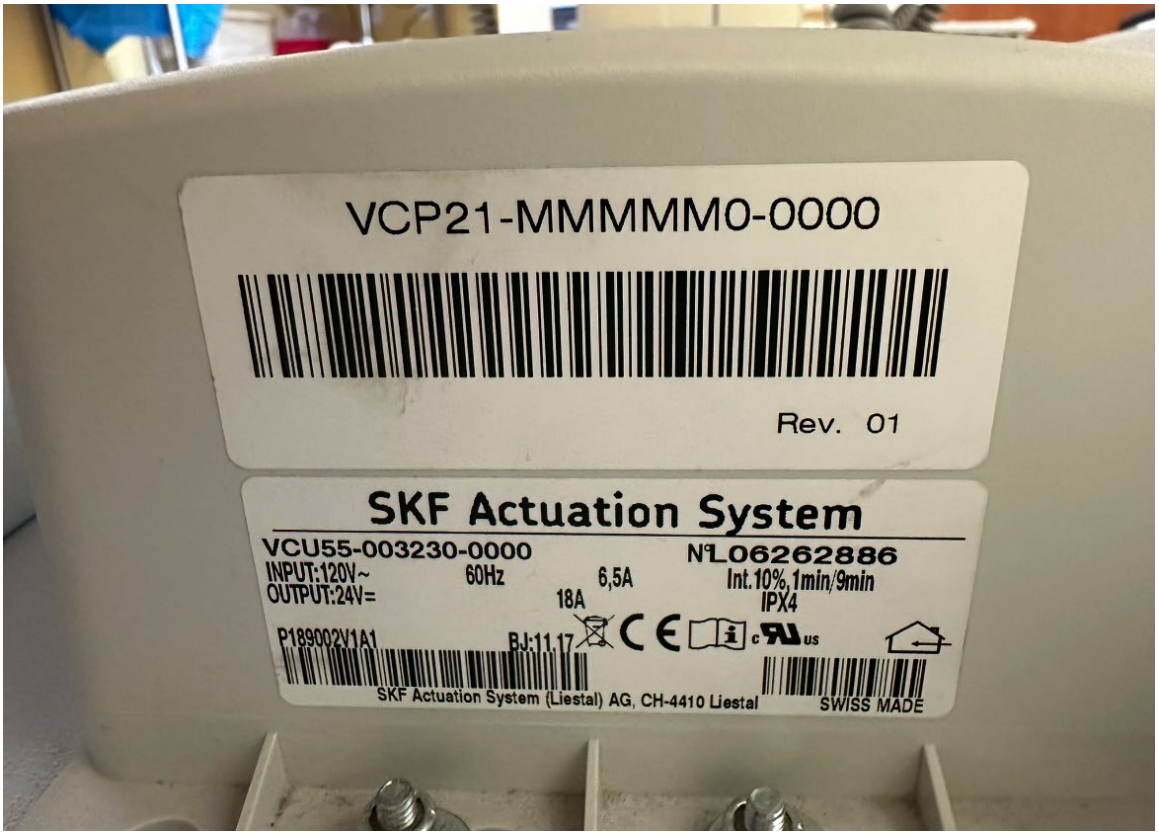

For VCU boxes we will need the VCP code also on the control box

VCU55 | Part Number: VCU 55-003230-0000

Heritage Medical Products, Inc.

SCU Boxes and SCP Code



For SCU boxes we will need the SCP code also on the control box

SCU56 | Part Number: SCU56-003230-0016

Inside of control box



Heritage Medical Products, Inc.

Power Cords

KOM Power Cord



For KOM control boxes

VCU and SCU Power Cord



For VCU and SCU control boxes

BCU Control Boxes have power cords built in.

If your power cord on a BCU box becomes damaged you must replace the entire box.



Heritage Medical Products, Inc.

Lift Columns




Regular Height Column | Part Number: TLG10-AA310-000


Low Column | Part Number: TLT10-A1410-000

CMPT | Part Number: CMPT-1S0500F2-000

Heritage Medical Products, Inc.

Actuators

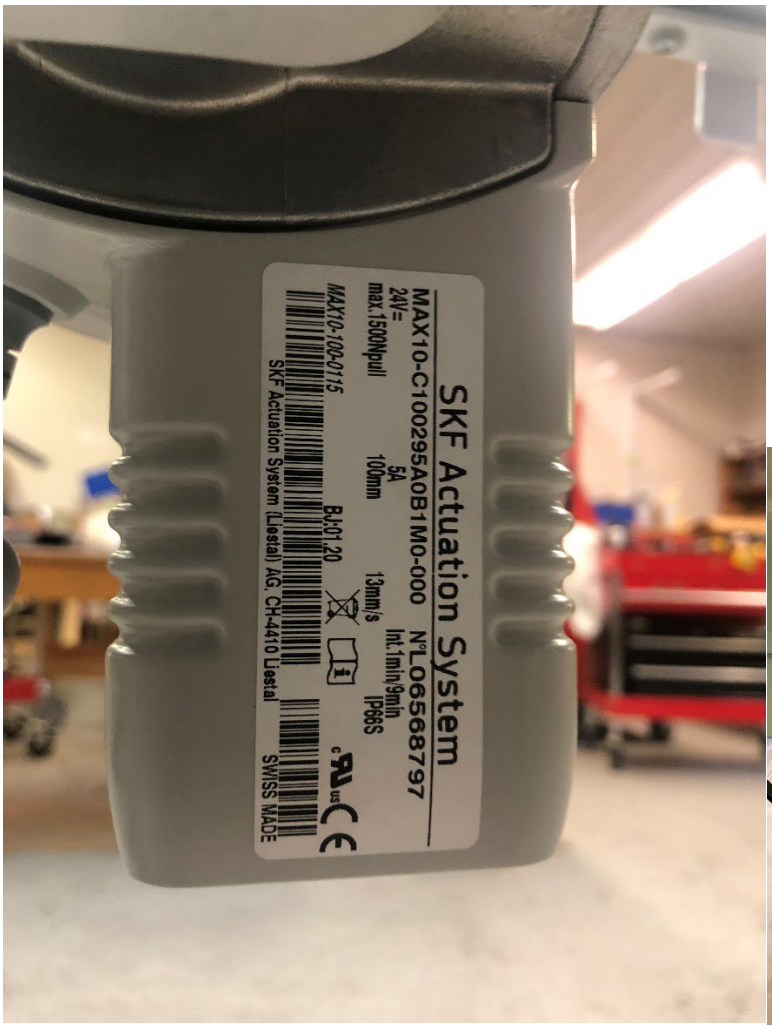

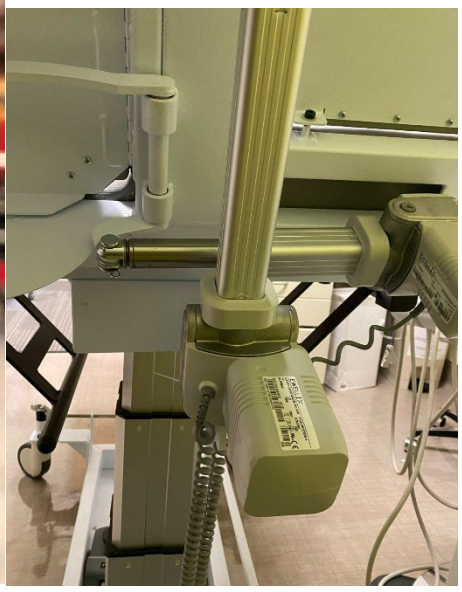

A loud, grinding sound is usually an indicator the actuator is going out.

Fowler Actuator | Part Number: MAX30-C200415A0A1MO-000

Drop Section Actuator | Part Number: MAX10-C100295A0B1MO-000

Wedge Section Actuator | Part Number: MAX10-C150345A0A1MO-000

Foot Section Actuator | Part Number: MAX10-C150345A0A1MO-000

Trendelenburg Actuator | Part Number: MAX10-C150345A0A1MO-000

Heritage Medical Products, Inc.

Foot Controls



Part number located on the back of the foot control.

1 Function Foot Control for VCU, BCU, SCU Boxes | Part Number: STJ01-LU1000-X100

2 Function Foot Control for VCU, BCU, SCU Boxes | Part Number: STJ02-LU1000-X101

3 Function Foot Control for VCU, BCU, SCU Boxes | Part Number: STJ03-LU1000-X102

4 Function Foot Control for VCU, BCU, SCU Boxes | Part Number: STJ04-LU1000-X102

1 Function Foot Control for KOM33 boxes | Part Number: STF01-LU1000-X100

2 Function Foot Control for KOM33 boxes | Part Number: STF02-LU1000-X100

3 Function Foot Control for KOM33 boxes | Part Number: STF03-LU1000-X100

4 Function Foot Control for KOM33 boxes | Part Number: STF04-LU1000-X100

1 Function Foot Control for KOM25 boxes | Part Number: STG01-LU1000-X100

2 Function Foot Control for KOM25 boxes | Part Number: STG02-LU1000-X100

3 Function Foot Control for KOM25 boxes | Part Number: STG03-LU1000-X100

4 Function Foot Control for KOM25 boxes | Part Number: STG04-LU1000-X100

Continued below

Heritage Medical Products, Inc.

Distribution Cord / Box Information for Foot Controls:

VCU55 Control Box -- no cord or box needed

BCU53 Control Box -- distribution cable needed

KOM33 Control Box -- distribution box needed

Casters

Individual Locking Casters: Plate Casters



Old style plate casters have been discontinued.

The new style plate casters (pictured above) is compatible with most of our beds. A higher quality caster that has performed better in the field.

Individual Locking Casters: Stem Casters



Central Locking Casters




If you need less than 4 central locking casters, we will need to know if they want the directional or non-directional central locking caster.

They are identical, but have different functions. The directional casters will be at the head of the bed and the non-directional casters will be at the foot of the bed.

Heritage Medical Products, Inc.

Paper Roll Holder



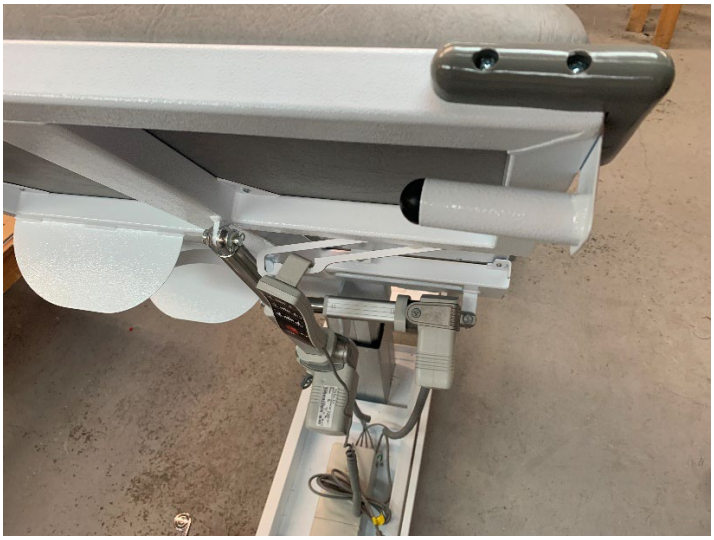

We sell 27" exam bed paper designed to fit the space of the built in paper roll holder. Paper rolls are available by the roll or in cases of 12 rolls.

If you'd like to use a different paper that is not as wide use the wooden dowel rod that came with the bed. (See picture below)



Take the black caps off the paper roll holder and put it in there with the paper of your choice.

Magnetic Hand Control Hanger

